


NEVER USE PIPE DOPE OR ANY OTHER LIQUEFIED PIPE SEALANT ON ANY CONNECTION IN A HIGH PURITY SYSTEM. ANY PIPE DOPE OR LIQUEFIED SEALANT CONTAINS CONTAMINANTS THAT WILL IMPACT YOUR ANALYSIS. ONLY USE TEFLON TAPE ON BRASS FITTINGS, THERE IS NO LUBRICANT REQUIRED. STAINLESS STEEL CONNECTIONS REQUIRE SPECIAL INERT LUBRICANTS FOR EITHER A HIGH PURITY OR ANALYTICAL SYSTEMS. ALL COMPONENTS OF OXYGEN SYSTEMS MUST BE COMPATIBLE AND APPROVED FOR OXYGEN SERVICE.

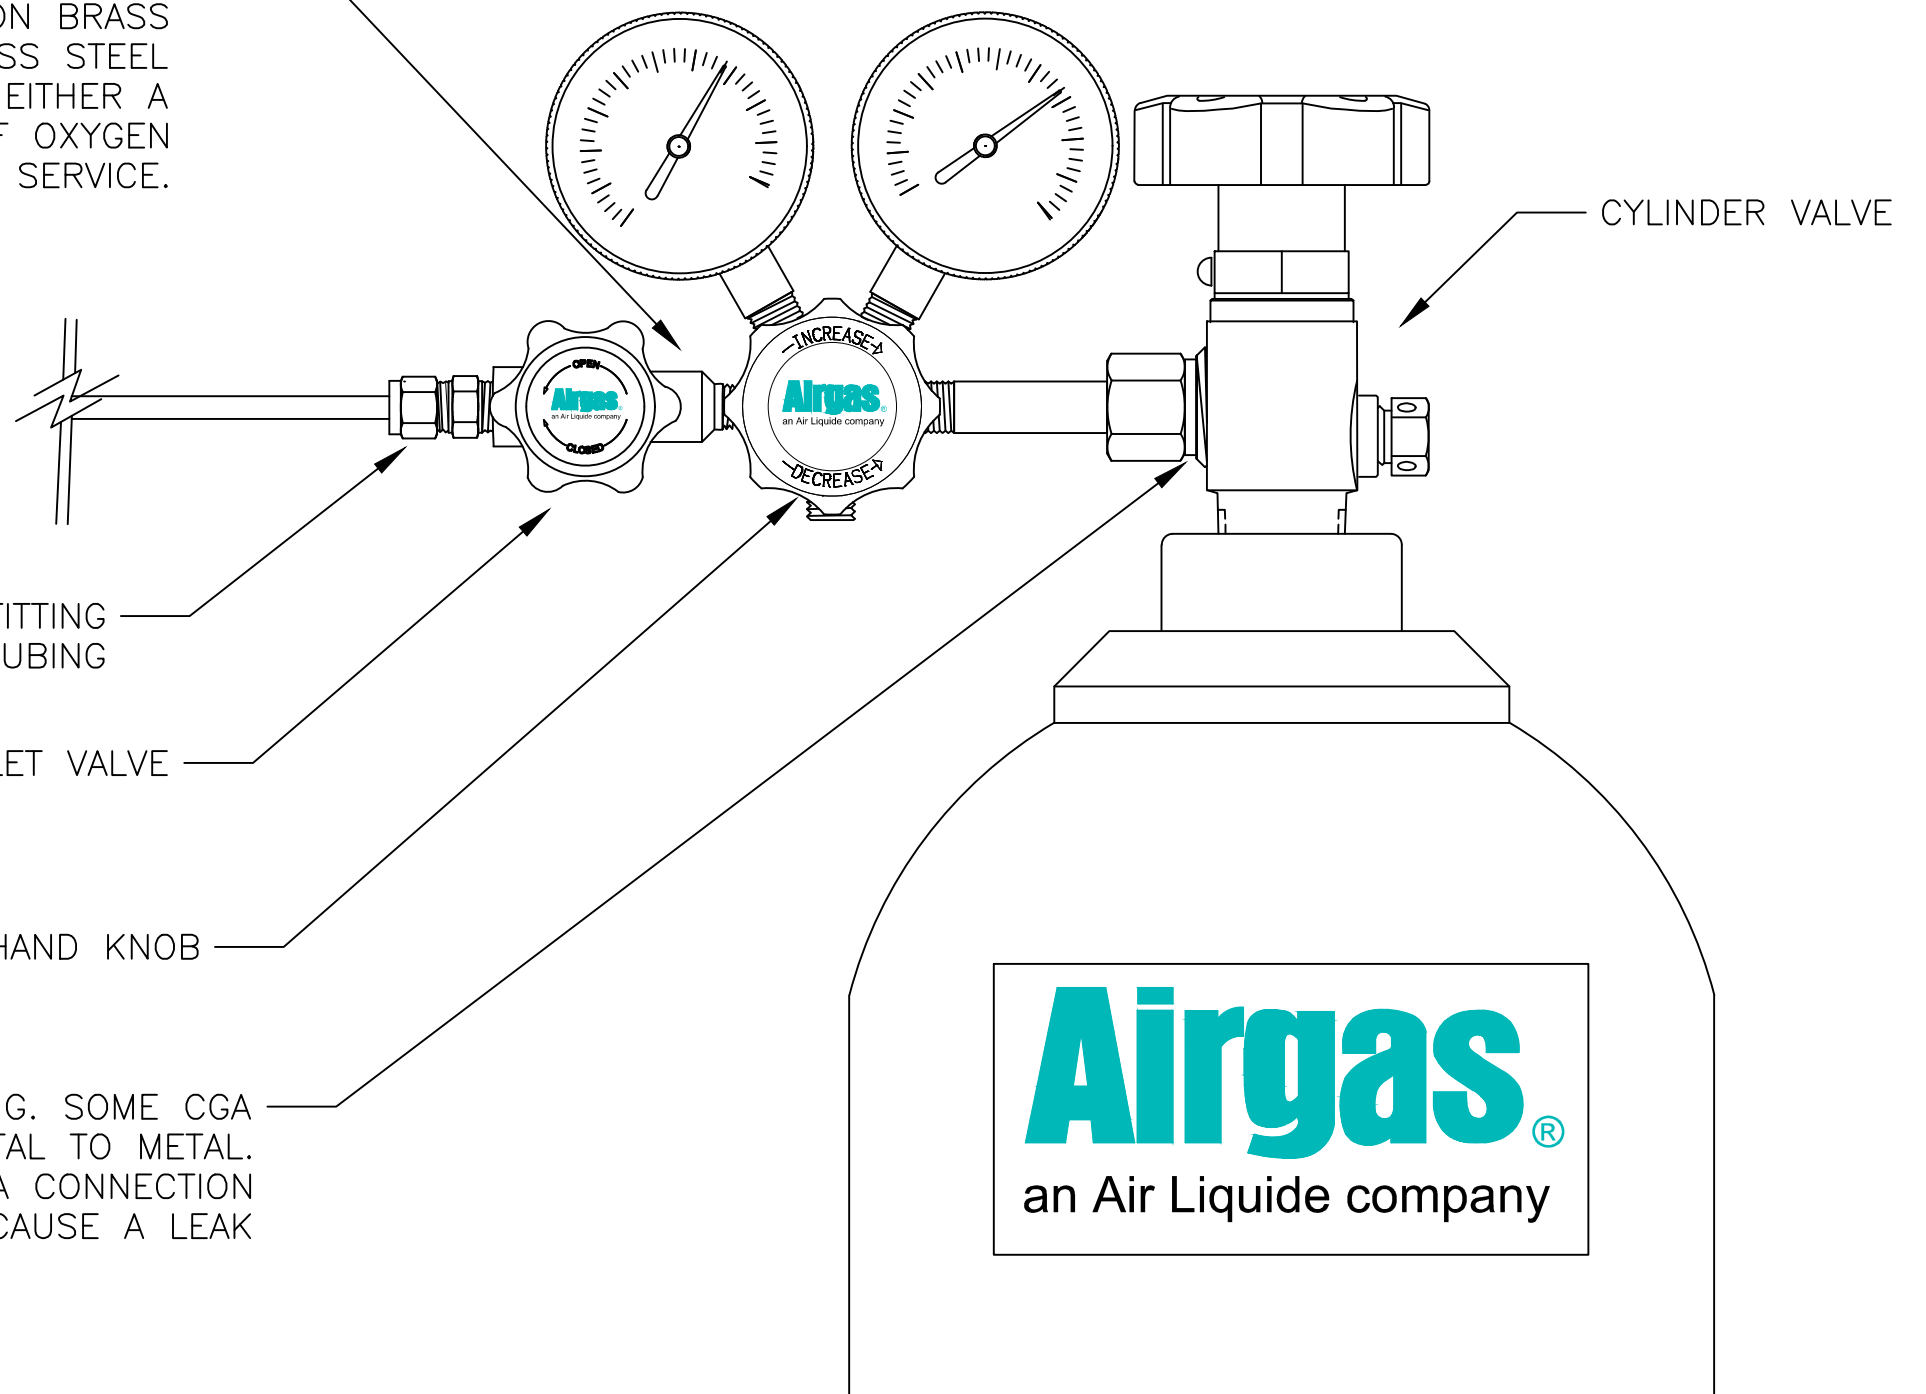

THE MATERIAL OF THE COMPRESSION FITTING MUST BE THE SAME AS THE TUBING

REGULATOR OUTLET VALVE

REGULATOR HAND KNOB

DO NOT USE TEFLON TAPE ON THE CGA FITTING. SOME CGA FITTINGS SEAL WITH A GASKET, OTHERS ARE METAL TO METAL. NEVER USE TEFLON TAPE TO SEAL A METAL CGA CONNECTION AS IT WILL CAUSE A LEAK



UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ON ANGLES $\pm 1^{\circ} 2'$ PLACES $\pm .03$ 3 PLACES $\pm .010$ INTERPRET DIN AND TOL PER ASME Y14.5 - 1994		CONFIDENTIAL NOTICE THIS DOCUMENT AND THE DESIGNS, SPECIFICATIONS AND ENGINEERING INFORMATION DISCLOSED HEREON ARE THE PROPERTY OF AIRGAS INC. AND ARE NOT TO BE DISSEMINATED OR REPRODUCED WITHOUT EXPRESS WRITTEN CONSENT OF AIRGAS INC. THIS PROPRIETARY DOCUMENT IS BEING SENT IN CONFIDENCE AND ONLY FOR CONSIDERATION OF THE MATTERS HEREON. IN ACCEPTING THE LOAN OF THIS DOCUMENT, RECIPIENT AGREES TO KEEP IT AND THE MATTERS DISCLOSED HEREON IN CONFIDENCE AND SHALL NOT USE THEM NOR PERMIT THEIR USE IN ANY WAY DETRIMENTAL TO AIRGAS INC.	Airgas [®] SPECIALTY GAS EQUIPMENT TAYLORS, SC an Air Liquide company
SCALE	SPECIALTY GAS EQUIPMENT GROUP	DRAWN BY MN	CH'KD BY FK
DATE 4/20/18	PIPE FITTING SEALANTS- WHERE IS IT OK TO USE		
SHEET NUMBER 1 OF 1	PROJECT NUMBER CUSTOM	DRAWING NUMBER REV. DATE DESCRIPTION APP. BY	

REV.	DATE	DESCRIPTION	APP. BY